

Figure 1

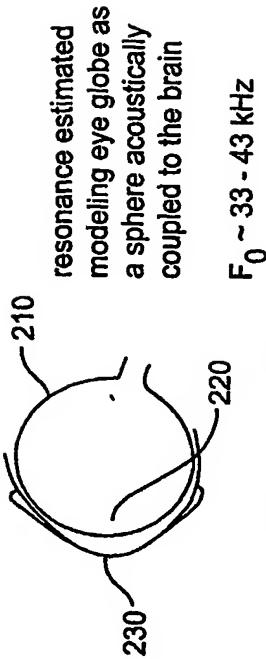


Figure 2A

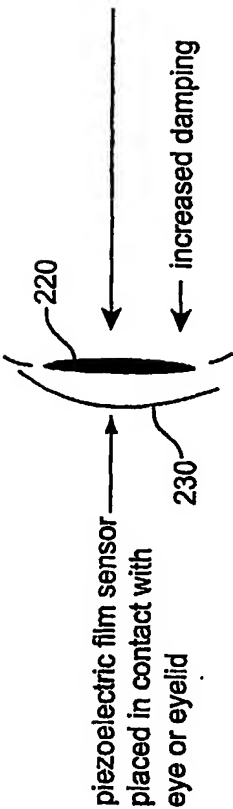


Figure 2B

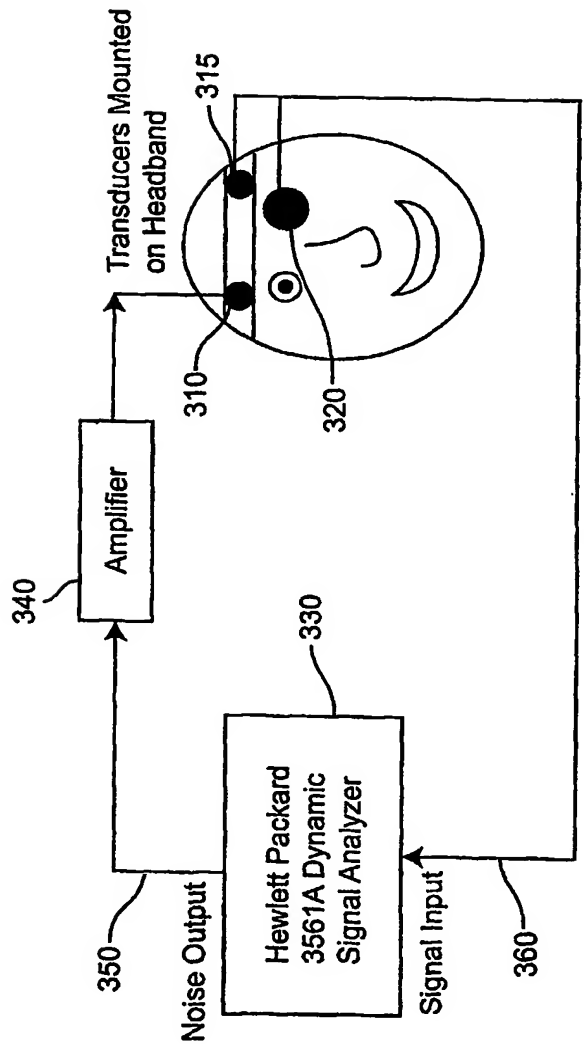


Figure 3

4/10

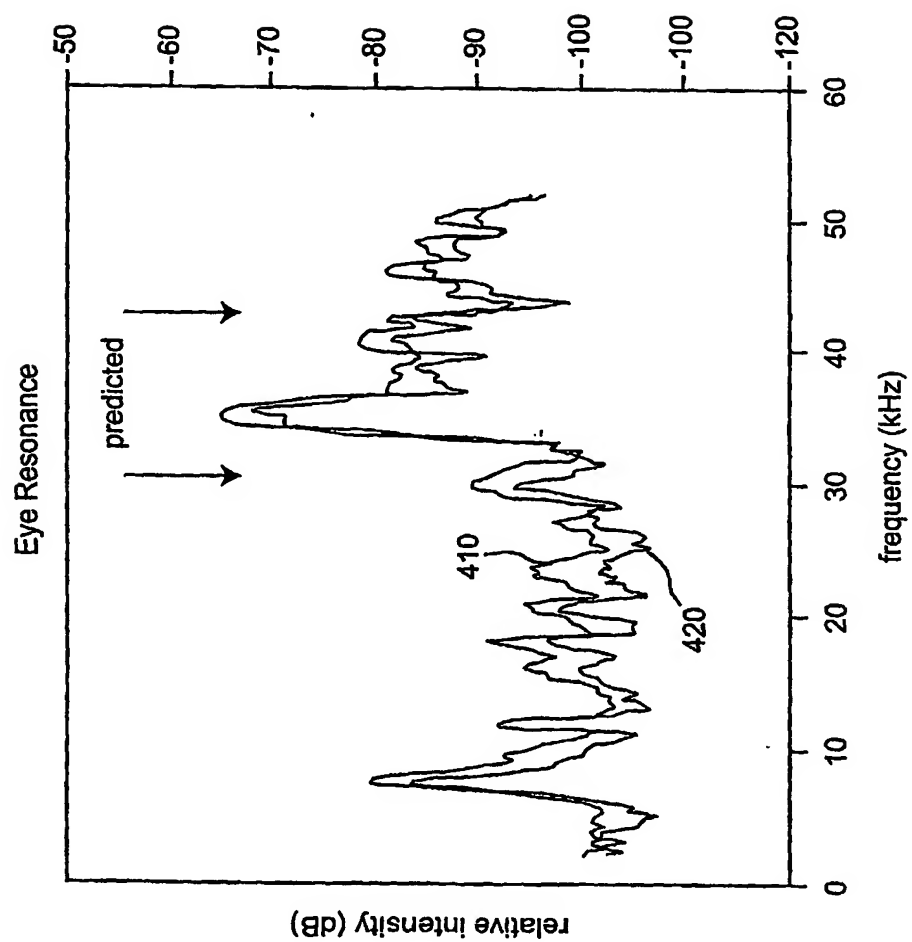


Figure 4

5/10

Direct ICP measurement (calibration)

| 510 | 520 | 530 |
|---------|----------------------------|-----------|
| Patient | Invasive Method Monitoring | ICP |
| HB | Ventriculostomy | 7 mm Hg. |
| GC | Ventriculostomy | 11 mm Hg. |
| GJ | Ventriculostomy | 15 mm Hg. |
| RR | Ventriculostomy | 20 mm Hg. |
| BP | Ventriculostomy | 18 mm Hg. |

Figure 5

6/10

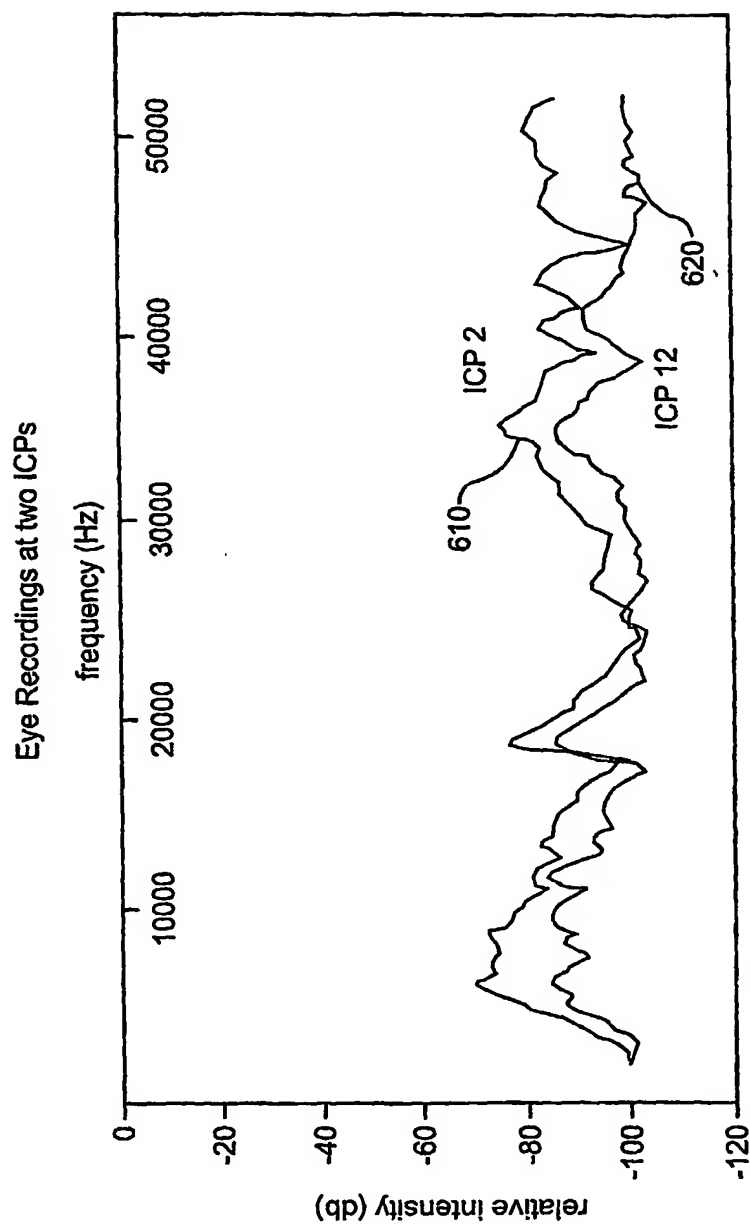


Figure 6

7/10

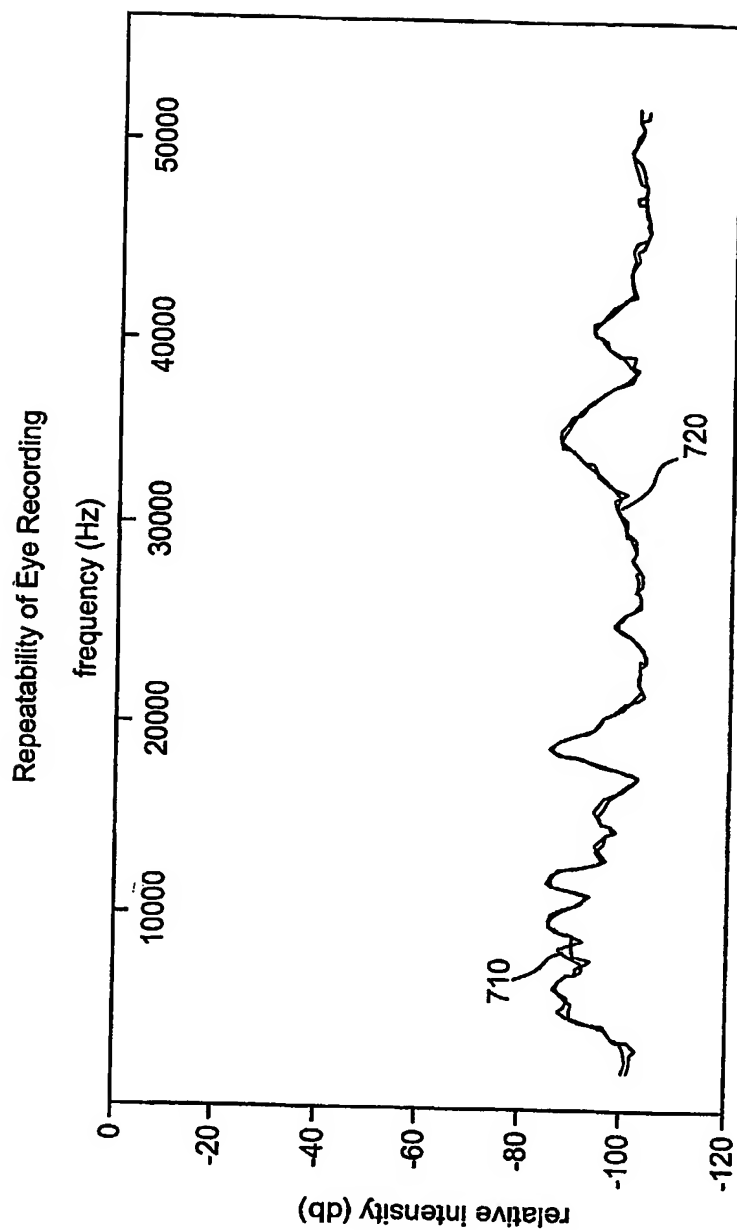


Figure 7

8/10

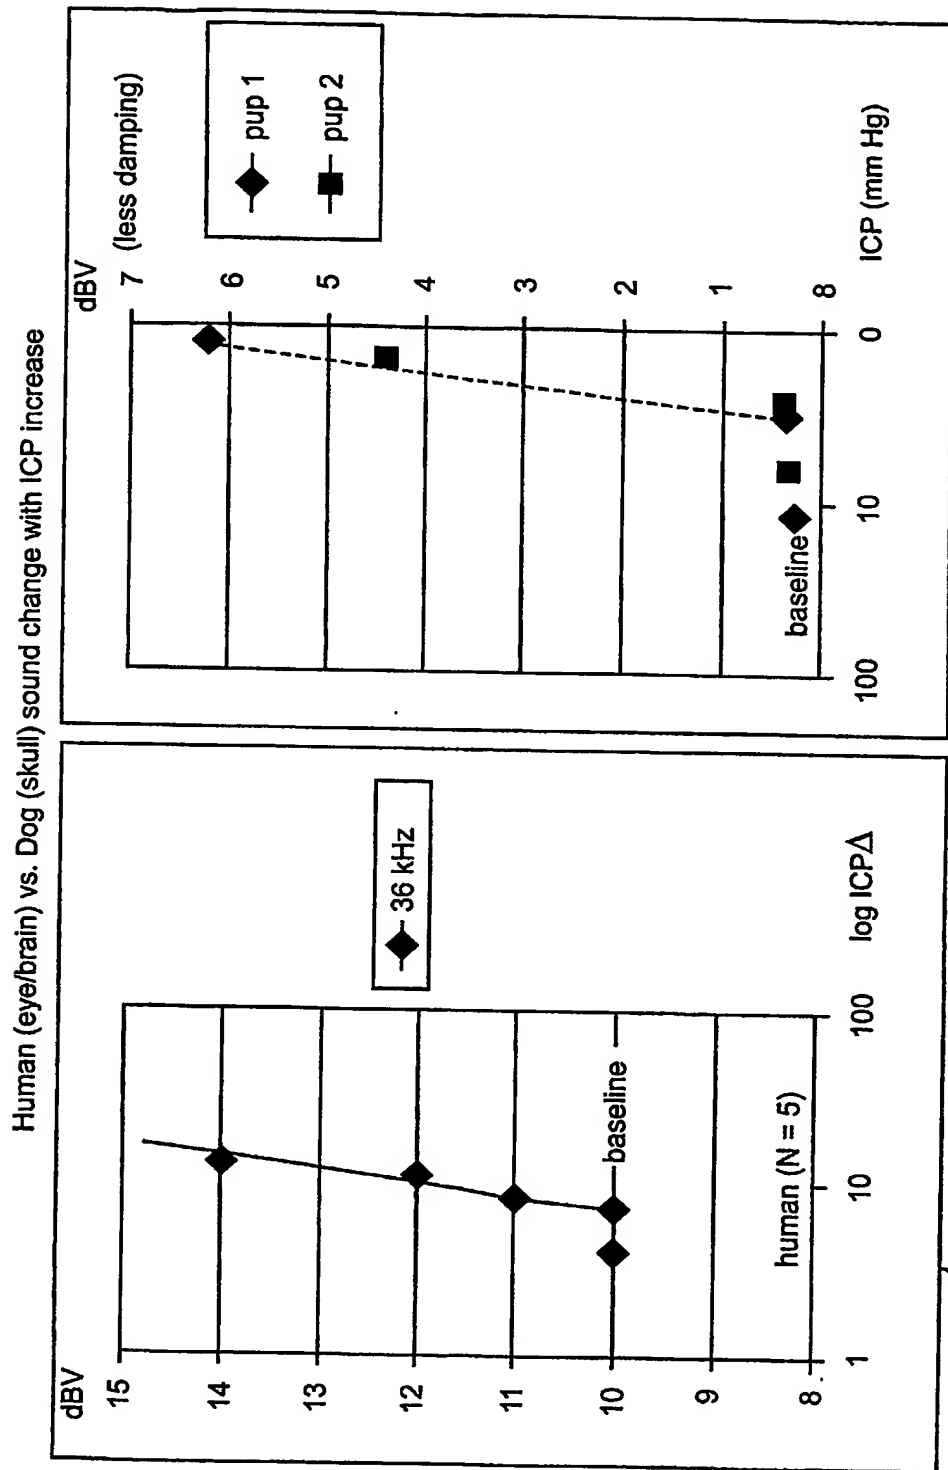


Figure 8

9/10

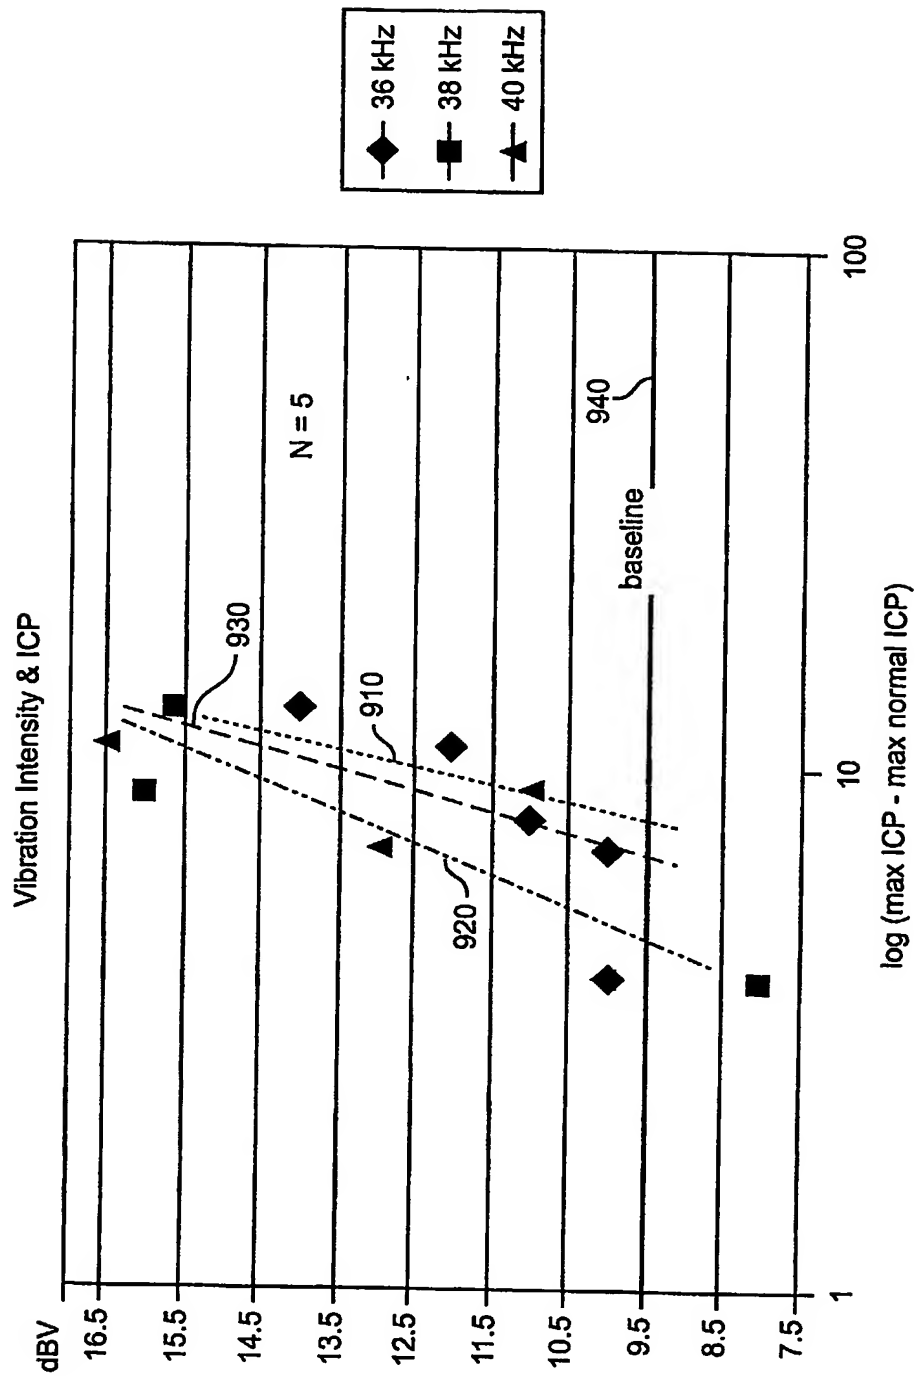


Figure 9

